




Results of OCIGO¹'s accuracy and repeatability tests in relation to the requirements of standards NF EN 16280 and NF EN 15964

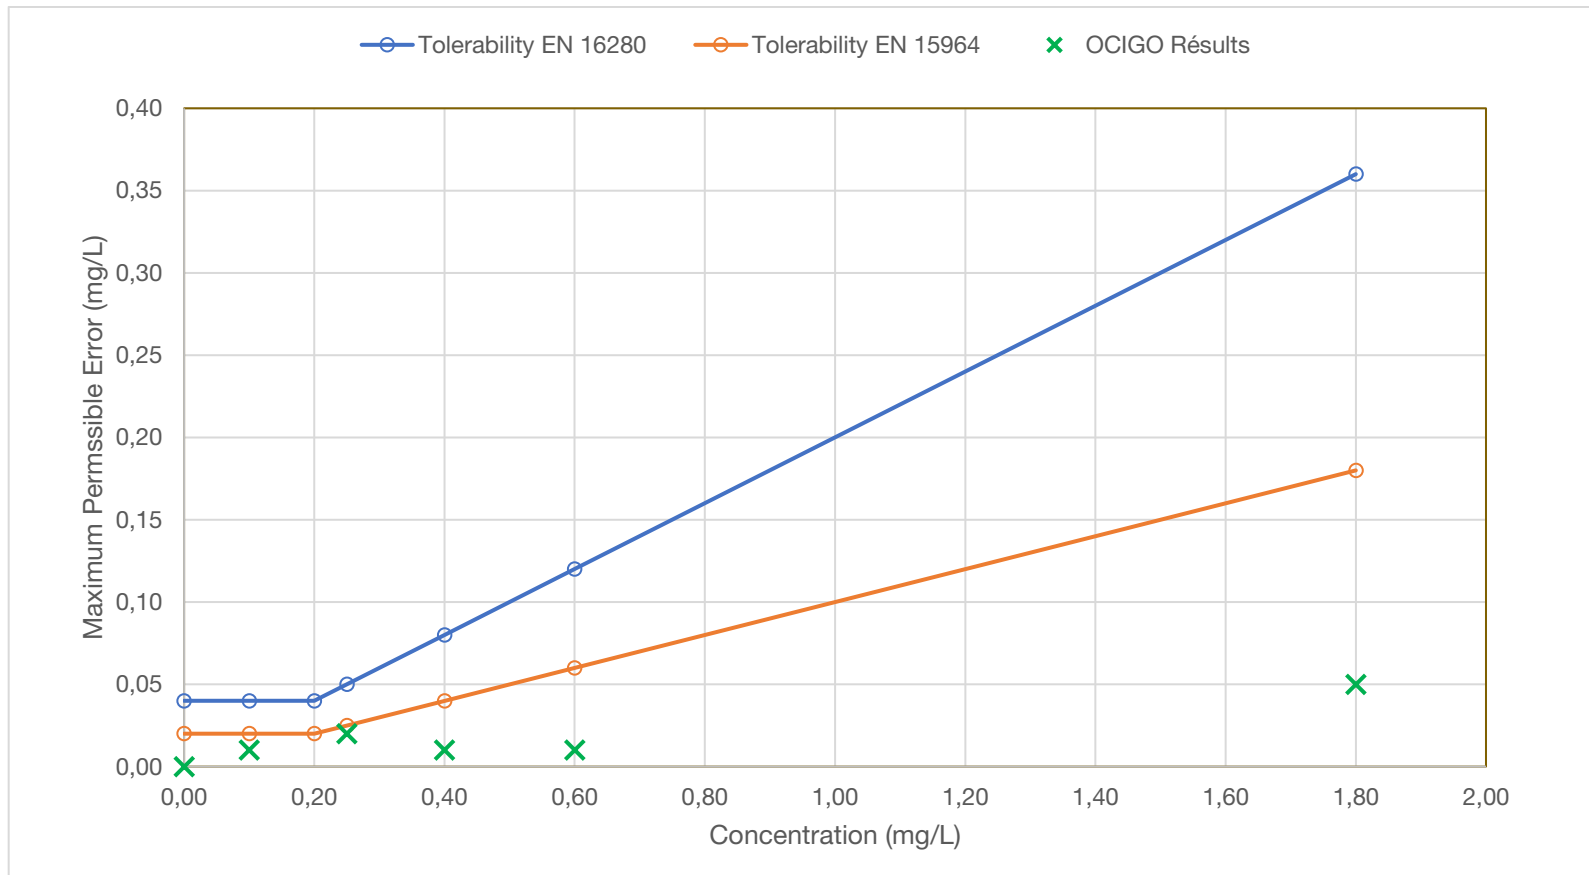

¹ Maximum errors found on an OCIGO tested by the National Testing Laboratory